



Prosthetic socket circumference at the very end of the cover in [mm]





To take the measurement correctly, please mark the height of the cover in several places and place a ruler below the marking. The measurement should be made very carefully because moving the ruler even by a few millimetres up or down causes an incorrect reading of the circumference even by several centimetres.



The height of the cover in [mm]



In the case of a parabolic foot shell, the height measurement must take into account the lowest point. In this case, the cover should be ground to the shape of the foot yourself.

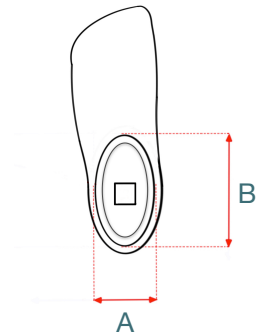


A [mm]

B [mm]

Foot manufacturer, type and size

For example : OB Taleo 1C50 L29



25 cm

45 cm

20 cm

40 cm

15 cm

35 cm

10 cm

30 cm

Adapter

☐ 30

☐ 34

Colour

☐ Skin Tone1

☐ Grey

☐ White

☐ Skin Tone3

☐ Black

☐ Skin Tone6

☐ Graphite

Finish

☐ Matt varnish  
( charged extra )

Tattoo ( charged extra )

☐ Catalog number from  
the our website.  
e.g.; 08-1001

☐ Own

Check list :

☐

Photo of the foot or shell.

Both the outer and inner edges of the shell contour must be visible. The camera lens must be perpendicular to the pyramid.


☐

4 photos,

as shown in the images above. The camera must be placed perpendicular to the legs, in a low position, and both legs must be centered on the photo. Please remember that all prosthetic components must be completely visible, including the socket. Please remove shoes, socks and any object that covers the prosthesis.




☐

Photo of the prosthesis with a measuring ruler applied.



☐

Photo of the prosthesis from the lateral.


Position the camera so the top of the foot shell looks like a straight line.

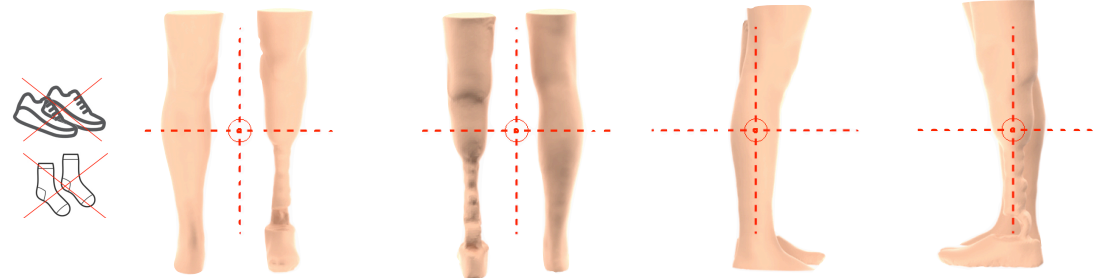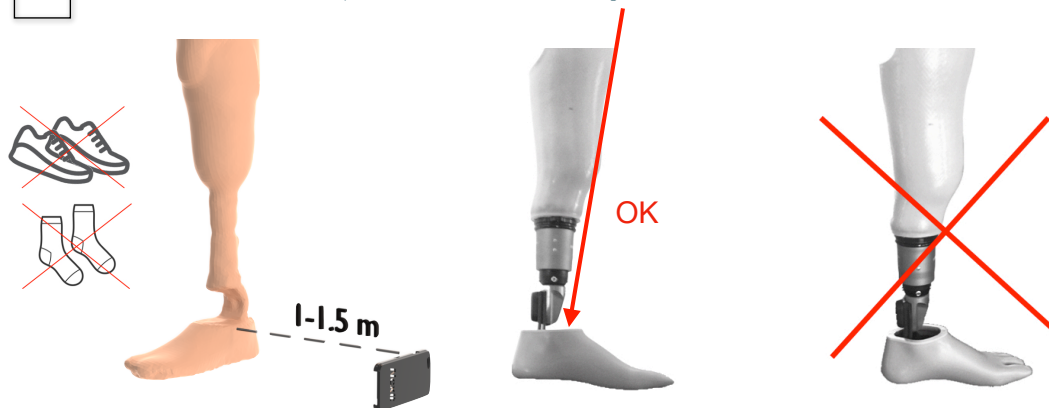

## NOTES

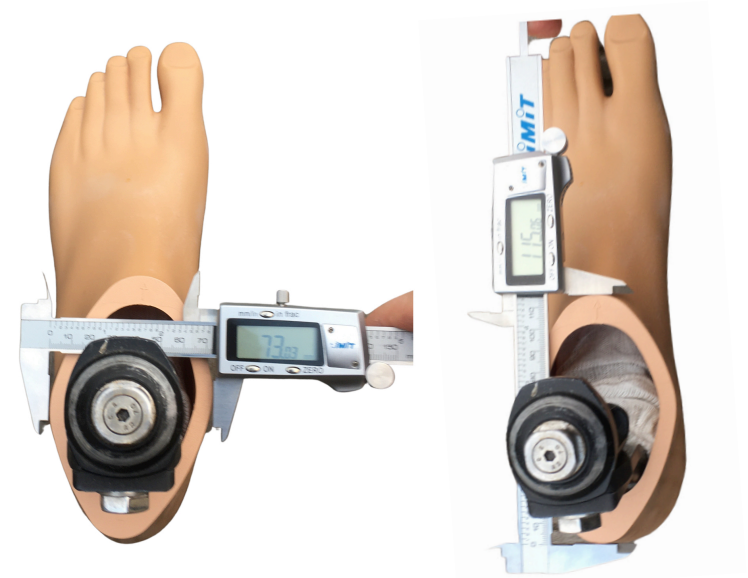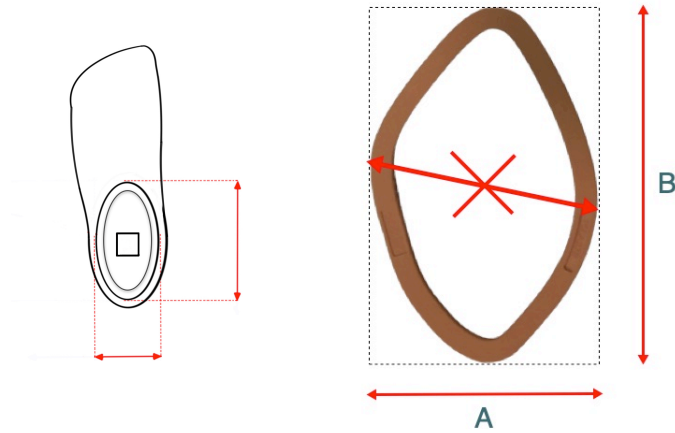

- Photo of the prosthesis with a measuring ruler applied.
- All photos are taken without shoes and socks!



- All our covers can be shortened from the bottom by several mm.
- In the factory state, the lower part of the cover is flat.
- In the case of the foot as shown in the picture, the lower part of the cover can be ground to the shape of the foot.
- If something is incomprehensible, look at our videos on the website in the menu - "VIDEOS"

